

Nano-communication for Biomedical Applications: A Review on the State-of-the-art from Physical Layers to Novel Networking Concepts

Qammer H. Abbasi, *Senior Member, IEEE*, Ke Yang, *Student Member, IEEE*, Nishtha Chopra, *Student Member, IEEE*, Josep Miquel Jornet, *Member, IEEE*, Najah Abed AbuAli, *Member, IEEE*, Khalid Qaraqe, *Senior Member, IEEE*, Akram Alomainy, *Senior Member, IEEE*

Abstract—Nano-communication based devices have the potential to play a vital role in future healthcare technologies by improving the quality of human life. Its application in medical diagnostics and treatment has a great potential, because of its ability to access small and delicate body sites non invasively, where conventional medical devices fall short. In this paper, the state of the art in this field is presented to provide a comprehensive understanding of current models, considering various communication paradigms, antenna design issues, radio channel models based on numerical and experimental analysis and network and system models for such networks. Finally, open research areas are identified for the future directions within the field.

Index Terms—nano communication, Terahertz, body area network, channel modeling, network modeling.

I. INTRODUCTION

In this era of envisioned unprecedented nanotechnology role in multidisciplinary domains such as environmental, industrial, biomedical and military; one of the emerging social and scientific impact of such technology would be in healthcare and bioengineering applications. As a promising alternative to current medical technologies like catheters and endoscopes, the nano enabled devices could reach to delicate body sites such as the spinal cord, gastrointestinal or inside the human eye, non invasively, which have not been possible yet with current technologies [1]. Due to the characteristics of iniquitousness and variety of the nano-devices, different kinds of information can be sensed and gathered together to complete complicated tasks. The connectivity and links between nano devices leads to the idea of nano-networks followed by the nano-communication proposal, which will expand the capabilities of these devices in terms of enhancement in features and

range of operations [2]. Among many types of communication between nano devices, one of the promising technique for the data exchange is Electromagnetic based communication at terahertz band [3]. This under utilised spectrum at the terahertz (THz) would significantly contribute to potential future medical technologies because of its less susceptibility to propagation effects such as scattering and its safety advantage for biological tissues *i.e.*, non ionization [4]. By using bio-nano-sensors in medicine, e-health monitoring system [5] can be realized, so is e-drug delivery systems [2] with the aid of nano-robots. The ultimate goal is to connect nano-network to the internet, by which and e-living and e-health can be fulfilled [6].

The evolution of novel materials such as graphene and carbon nano tubes (CNT) [7], which can work at THz frequencies opens up new opportunities of applying these nano-devices inside the body. In recent years, body-centric communication has been studied for a wide range of frequencies [8], [9], however the size reduction requirements make nano-scale technologies an attractive choice for future applications of body-centric communication. Due to short wavelength, even a minute variations in water contents and biomaterial tissues can be detected by terahertz radiations due to existence of molecular resonances at such frequencies. Consequently, one of the emerging areas of research is analysing the propagation of terahertz electromagnetic waves through the tissues to develop diagnostic tools for early detection and treatment such as abnormalities in skin tissues as a sign of skin cancer [10]. Although there are some limited studies in open literature with regards to nano-communication and applicability of THz communication in the biomedical domain [1], [5], [11]–[16]. All published studies are scattered with none encompassing all aforementioned issues. In this paper, we are presenting a comprehensive state-of-the-art review of nano-communication with emphasis on biomedical applications and discussion on several research challenges by considering various communication methods, antenna design considerations, channel modeling aspects, while highlighting various simulation issues and measurement techniques in addition to network and system models.

The rest of the paper is organized as follows. Section II highlights the envisioned applications for nano communication and proposed network architecture for healthcare applications. Section III details brief discussion about various paradigms of

This publication was made possible by NPRP grant # 7-125-2-061 from the Qatar National Research Fund (a member of Qatar Foundation). The statements made herein are solely the responsibility of the authors.

Qammer and Khalid are with the Dep. of Electrical and Computer Engineering, Texas A & M University at Qatar. Qammer is also with Queen Mary University of London and UET, Lahore.; e-mail: {qammer.abbasi;k.qaraqe}@tamu.edu.

Nishtha Chopra, Ke Yang and A. Alomainy are with Antennas & Electromagnetics School of Electronic Engineering and Computer Science Queen Mary University of London, London; e-mail: {n.chopra,ke.yang;a.alomainy}@qmul.ac.uk.

Najah Abed AbuAli is with College of Information Technology. United Arab Emirates University; e-mail:najah@uaeu.ac.ae

Josep Miquel Jornet is Department of Electrical Engineering, University at Buffalo, New York; e-mail:mjornet@buffalo.edu

communication among nano devices. Section IV presents an overview of different types of nano antennas while Section V details some of the state-of-art in nano devices from biomedical prospective. Section VI highlights the channel characterization at nano scale based on simulation and measurements at terahertz frequencies. Section VII presents the network and system model while open research areas are presented in Section VIII. Finally, conclusions are drawn in Section IX.

II. ENVISIONED APPLICATIONS AND THE NETWORK STRUCTURE

Nanonetworks have broad range of applications and can be mainly divided into four groups: environmental, biomedical, military and industrial [2] [5] as shown in Fig. 1.

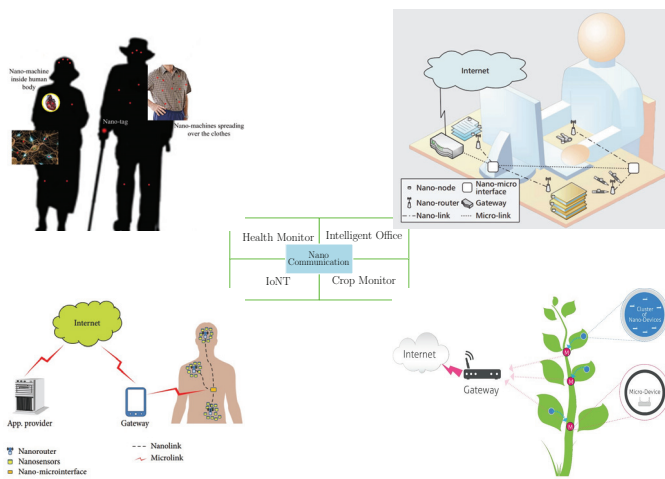


Fig. 1: Envisioned applications for nano communication (reproduced from [5])

Detailed description of the envisioned applications have been summarised and classified in [2], as shown in Tab. I. The table clearly shows that one of the most attractive application of nano-networks is in the biomedical fields due to its advantages of size, bio-compatibility and bio-stability. Nano devices spreading over the human body can monitor the human physical movement. For example, nano pressure-sensors distributed in the human eyes can detect the intraocular pressure (IOP) for the early diagnosis and treatment of glaucoma to prevent vision loss [1]. At the same time, the nano devices deployed in the bones can monitor the bone-growth in young diabetes patients to protect them from osteoporosis [1]. Furthermore, nano-robots inside the biological tissues can detect and then eliminate malicious agents or cells, such as viruses or cancer cells, hence making the treatment less invasive and real time [17]. Moreover, networked nano-devices will be used for organ, nervous track, or tissue replacements, *i.e.*, bio-hybrid implants.

Similar to the traditional body-centric communication, the nano network can also be divided into three parts: in-body, on-body and off-body. An overview of the structure of nano-network for healthcare domain as shown in Fig. 2 can be summarized as [6]:

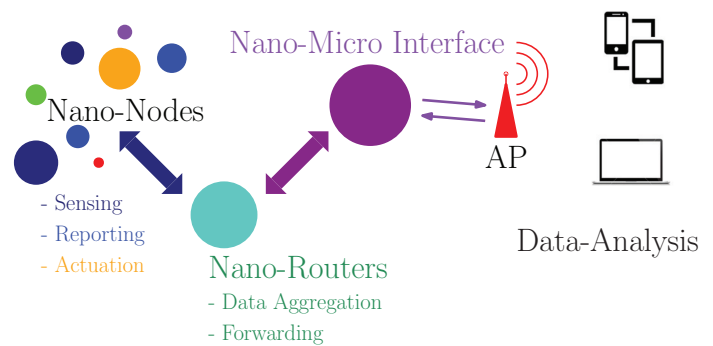


Fig. 2: Envisioned architecture for nano-healthcare

- **Nano-nodes:** These are the smallest and simplest nano-devices. Due to the limited energy, limited memory and reduced communication capabilities, they can only perform simple computation task and can transmit over very short distances. The nodes could be composed of sensor and communication units.
- **Nano-routers:** These are the nano-devices with slightly larger computational resources than nano-nodes and can aggregate information from limited nano-machines and also can control the behaviour of nano-nodes by sending extremely simple order (such as on/off, sleep, read value, *etc.*). However, this would increase their size; thus, their deployment would be more invasive.
- **Nano-micro interface:** They are used to collect the information forwarded by nano-routers and send the information to the micro-scale devices. At the same time, they can send the information from micro-scale to nano-scale. Nano-micro interfaces are hybrid devices not only able to communicate in the nano-scale using the nano-communication techniques shown in Section III but also can use classical communication paradigms in micro/macro communication networks.
- **Gateway:** It makes the users to control or monitor the entire system remotely over the Internet.

III. VARIOUS PARADIGMS OF NANO-COMMUNICATION

According to Akyildiz *et al.* [2], nano-communication can be divided into two scenarios: (i) Communication between a nano-machine and a larger system such as micro/macro-system, and (ii) Communication between two or more nano-devices. These devices can communicate by different mechanism like electromagnetic, acoustic, nanomechanical or molecular [50] *etc.*, which will be briefly discussed in this section.

A. Molecular Paradigms

Molecular communication are considered as the most promising paradigm in the start of nano era to achieve the nano-communication because there are numerous examples present in nature to learn and study. In molecular communication, an engineered miniature transmitter releases small particles into a propagation medium, while the molecules are applied to encode, transmit, and receive information. Molecular

TABLE I: Overview of the envisioned applications [1], [2]

	Biomedical [18]	Environmental	Industrial	Military
Health Monitor	<ul style="list-style-type: none"> • Active Visual Imaging for Disease Diagnosis [19] [20] [21] [22] [23] • Mobile Sensing for Disease Diagnosis [24] [25] [26] [27] 	Bio-Degradation [5]	Product Quality Control [28]	Nuclear, Biological and Chemical Defences [29]
Therapy	<ul style="list-style-type: none"> • Tissue Engineering [30] [31] [32] • Bio-Hybrid Implant [33] [34] • Targeted Therapy/Drug Delivery [35] [36] [37] [38] [39] • Cell Manipulation [40] [19] [41] [42] [43] • Minimally Invasive Surgery [44] [45] [46] 	Bio-Control [47] [48] [49]	Intelligent Office [6]	Nano-Fictionalized Equipment [50]

communication can be classified into several categories such as walkway-based: molecules propagate along a predefined pathway via molecular motors; flow-based: molecules propagate in a guided fluidic medium; diffusion-based: where molecules propagate in a fluidic medium via spontaneous diffusion and *etc.* [5]. The diffusion-based molecular communication (DMC), the most general and widespread scheme found in nature is most widely investigated in the literature. Some of the most prominent works include mathematical framework for a physical end-to-end channel model for DMC [51], development of an energy model for DMC [52], modeling of diffusion noise [53], channel codes for reliability enhancement [54], and relaying-based solutions for increasing the range of DMC [55], [56]. On the other hand, the flow-based molecular communication (FMC) is also studied, especially the one of communication in the circulatory system [57], [58].

B. Acoustic Paradigm

Acoustic propagation introduces slight pressure variations in the fluid or solid medium, which satisfy the wave equation. The behaviour of the nano robots is relevant to their physical properties, surrounding medium and the working frequency. The feasibility of in vivo ultrasonic communication is evaluated by Hogg *et. al.* [59], where communication effectiveness, power requirements and effects on nearby tissue were examined on the basis of discussion on the principles. Later, the nanoscale opto-ultrasonic communications in biological tissues was discussed in [17], [60], where the generation, propagation model were studied and in line with [59] the hazards and design challenges were investigated.

C. Touch Communication Paradigm

Based on the development of the nanotechnology, a new paradigm of touch communication (TouchCom) ¹ was also proposed in [57], which use a swarm of nano-robots as message carrier for information exchange. In TouchCom, transient microbots (TMs) [61]–[63] were applied to carry the drug particles, which can be controlled and tracked by the external macro-unit (MAU) with a guiding force [58], [64]. These TMs would survive some time in body and their pathway would be the channel for the information exchange while the process of loading and unloading is the corresponding transmitting and receiving process. A specific application, illustrated in [57], was shown in Fig. 3 while the structure of the applied nano-robots was shown in Fig. 4. The channel model of TouchCom was derived by defining the propagation delay, path loss with

¹Here, touch means the communication (*i.e.*, drug delivery) process is controllable and trackable.

the angular/delay spectra of the signal strength. Meanwhile, a simulation tool was proposed to characterize the movement of the nano-robot swarm in the blood vessel.

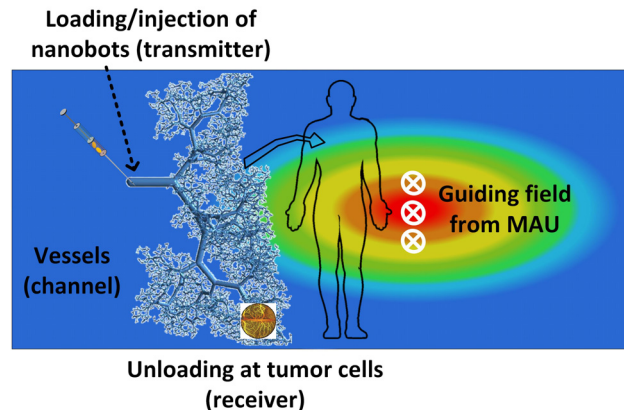


Fig. 3: Envisioned TouchCom system [57]

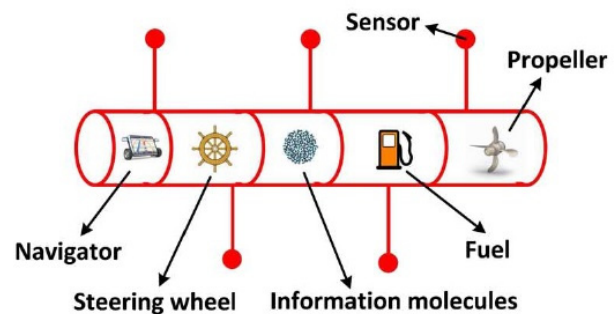


Fig. 4: Structure of the envisioned nano-robots [57]

D. Electromagnetic Paradigm

As the name indicates, electromagnetic methods use the electromagnetic wave as the carrier and its properties like amplitude, phase, delay *etc.* are used to encode or decode the information. The possibility of EM communication is first discussed in [5] on the basis of the fact that terahertz band can be used as the operational frequency range for future EM nano-transceivers because of the emerging new materials like Carbon Nano-Tube (CNT) and Graphene [65]. In [66] the theoretical model of the nano-network whose nodes are made of CNT was presented. Later, the channel model for THz wave propagating in the air with different concentration of the water vapor was presented in [15] and the corresponding

channel capacity was also studied. Based on the characteristics of the channel, a new physical-layer aware medium access control (MAC) protocol, Time Spread On-Off Keying (TS-OOK), was proposed in [67]. Meanwhile, the applications of THz technology in imaging and medical field [11], [12] has also achieved great development and the biological effects of THz radiation are reviewed in [16] showing minimum effect on the human body and no strong evidence of hazardous side effects. The focus of this review paper is on EM paradigm and in next sections, the paper will be confined only to discussions related to this paradigm.

IV. RECENT DEVELOPMENT IN NANO-ANTENNAS

Despite numerous studies on nano-technology are being published every year, however enabling the communication between nano-devices is still a major challenge, which is mainly related to the development of nano-antennas and the corresponding electromagnetic transceiver. Reducing the size of the traditional antenna down to a few hundreds of nanometers would lead to extremely high operating frequencies, which compromises the feasibility of electromagnetic wireless communication among nano-devices. Nano-antenna can be made of either conventional material *i.e.* metal or novel materials like carbon nanotube and graphene. This section is dedicated to give brief description about these two types of nano-antennas.

A. Metallic material based nano-antennas

There are different types of metal based nano antennas available in literature. Metallic plasmonic nano-antenna is one of the metallic material based nano-antennas presented in [68] for intra-body nano-networks. A unified mathematical framework was developed in this work to investigate the performance in reception of gold-based nano-dipole antennas. The analytical model shown in Fig. 5 was validated by COMSOL Multiphysics simulations.

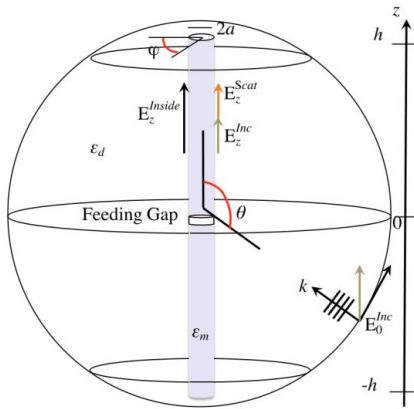


Fig. 5: Simulation results for the network.

Another kind of metallic material antenna is the optical metallic nano dipole antenna as presented in [69]. Five metals (silver, aluminium, chromium, gold, and copper) were compared, where the correspondence of the antenna length to

the working band was studied. Also, an in-house developed Method of Moments (MoM) based electromagnetic solver was developed to conduct this study. The results show that it is much more crucial to choose the proper metal in terms of operational frequency band for nano-antenna than the traditional ones. Besides the above general metallic nano-antennas, metal oxide metal (MOM) techniques was also applied for nano-antenna array [70] because of the excellent tunnelling characteristics.

B. Nano-antennas made of novel materials

The new materials like carbon nanotube and graphene are attractive choice for nano-antennas. It has been proved that above mentioned limitation like size and communication constraints, can be overcome by using the graphene to fabricate the antennas because the wave propagation velocity in CNTs and graphene nanoribbons (GNRs) can be up to one hundred times below the speed of light in vacuum depending on the structure geometry, temperature and fermi energy [71], leading to the fact that the resonant frequency of nano-antennas based on graphene can be up to two orders of magnitude below that of nano-antennas fabricated with other materials. Recent studies has already proved that CNT/graphene antenna can work at the THz band (*i.e.*, 0.1 - 10 THz); thus, the band of interest is the most promising candidate for the EM communication [5], [65], [72]. The CNT antenna was compared with classical dipoles by numerical analysis [73], while the possibility of CNT as dipole antenna was discussed, giving a mathematical framework [74]. [75] first demonstrated the performance of the propagation of EM waves on a graphene sheet. GNR-based nano patch antenna and CNT-based nano dipole antenna were compared in [76], showing that graphene-based antenna with the length of 1 μm can radiate EM wave at THz band, which agreed with the prediction in [77].

A beam reconfigurable multiple input multiple output (MIMO) antenna system based on graphene nano-patch antenna is proposed in [78], the radiation directions of which can be programmed dynamically, leading to different channel state matrices. For the short range communication, the proposed MIMO antenna design can enlarge the channel capacity by both increasing the number of antennas and choosing the best channel state matrices. An equilateral triangular patch antenna and rectangular patch antenna were designed using graphene as the patch conductor in [79], [80]. A log-periodic toothed nano-antenna based on graphene was proposed in [81]. Large modulation of resonance intensity in log-periodic toothed nano-antenna can be achieved via turning the chemical potential of graphene.

A novel graphene-based nano-antenna as shown in Fig. 6, which exploits the behaviour of Surface Plasmon Polariton (SPP) waves in semi-finite size Graphene Nanoribbons (GNRs) was proposed in [82]. By exploiting the high mode compression factor of SPP waves in GNRs, graphene-based plasmonic nano-antennas are able to operate at much lower frequencies than their metallic counterparts.


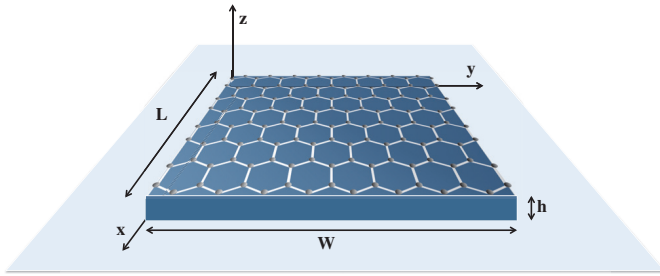



Fig. 6: A plasmonic nano-patch antenna based on graphene [82].

V. CURRENT DEVELOPMENT OF NANO-SCALE DEVICES

This section details about some of the state-of-the-art for nano devices in biomedical domain. Due to the developments in micro-fabrication and nano-technologies, the limits of the sizes and capabilities of devices have been pushed further. A cheap Integrated Chip (IC), whose cost would be less than one dollar, was designed by National Applied Research Laboratories, Taiwan using sensor fusion technologies, shown in Fig. 7a, which is smaller than a grain of rice. A full-duplex transceiver IC, shown in Fig. 7b was presented from Clumnia High-Speed and mm-wave IC Lab (CoSMIC) [83] in 2015, which was even further smaller.

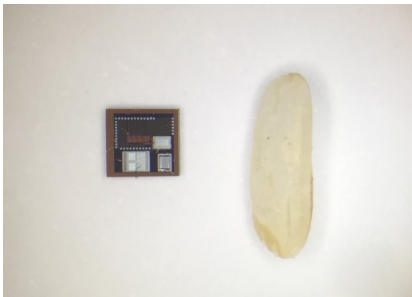

(a) Comparison of the chip with a rice (reproduced from [84])

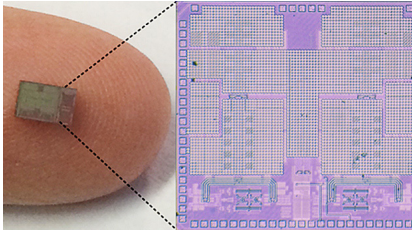


(b) Photo of the full-duplex transceiver IC ©CoSMIC Lab


Fig. 7: The Realized IC chips

The initial goal of developing small-scale devices is to replace the existing tethered medical devices such as flexible endoscopes and catheters because such devices could access complex and small regions of the human body like gastrointestinal (GI), spinal cord, blood capillaries and at the same time the discomfort and the tissue loss because of sedation would be hugely decreased. The micro-robots voyaging around human body were developed recently according to same principles. For example, a tiny permanent magnet, guided inside the


human body by a magnetic stereotaxis system was proposed in [85] while a magnetically driven screw were made to move through tissues [86]. Micro-mechanical flying insect robots were first created in University of California, Berkeley [87] and then later a solar-powered crawling robot was realized in [88]. The first medical-used capsule endoscopes, to replace the traditional ones, were applied clinically in 2001 with the FDA's approval. Later the introduction of a crawling mechanism [89] and on-board drug delivery mechanism [90] were marked as another milestone for the development of the capsule endoscopy. A nano-scallop capable of swimming in biomedical fluids whose size is only a fraction of a millimetre has been developed at the Max Planck Institute for Intelligent Systems [91], shown in Fig. 8a and at the same time a tiny bio-bot powered by skeletal muscle cells, shown in Fig. 8b was reported in [92]. A magnetic helical micro-swimmer was successfully targeted in a wireless way to deliver a single-cell gene to human embryonic kidney whose SEM image is shown in Fig. 8c [93].

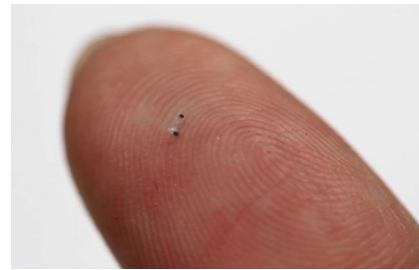

(a) Nano-scallop which can swim in bio-fluids (reproduced from [91])

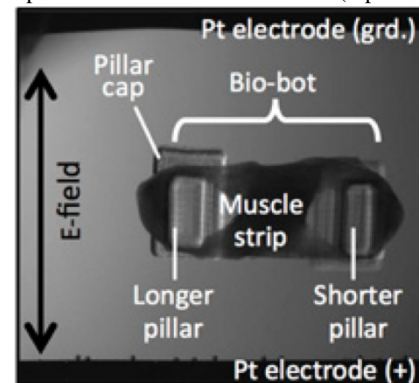

(b) Bio-bot powered by skeletal muscle cells ©UIUC

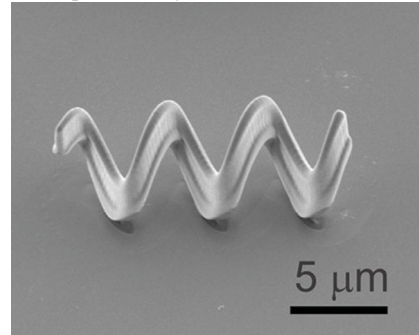

(c) SEM image of the artificial bacterial flagella (reproduced from [93])

Fig. 8: Photos of the nano-bots which can be used in human body

Besides the research activities on tiny robots, there are also investigations on other applications. A wireless radiation detector was designed to inject into the tumour to detect the level of the therapeutic radiation the tumour gets [94]. Applying micro-machining techniques, this dosimeter was shrunk to 2 cm long and 2 mm wide in diameter.

VI. CHANNEL MODELING FOR NANO SCALE COMMUNICATION AT TERAHERTZ FREQUENCIES

In order to fully exploit and increase further the potential of nano devices in biomedical applications, the EM waveforms propagation and accurate channel models knowledge inside the body is necessary, which are vital to build efficient, reliable and optimized high performances systems. It is essentially important to create and access such a models for achieving target link budgets, high data rates and designing efficient transceivers and antennas including digital baseband algorithms. Because of the limitations such as size, complexity and energy consumption, EM communication between nano-devices have been considered very challenging initially [95]. However, with the advent of the carbon-based materials like graphene and CNT, attention has been moved to the EM communication [5], [66] slowly.

With consideration that the communication is at nanoscale, the study of the communication between very short range is essential [15], [96]. Jornet *et al.* presented a modified Friis formula for pathloss calculation [15] in water vapor at THz, which has two parts: the absorption path loss and the spread path loss. Later, a more detailed model of THz communication is proposed with the consideration of multi-ray scenario; thus, the propagation models for reflection, scattering and diffraction is considered [97]. At the same time, the scattering effects of small particles was discussed with the frequency analysis and the impulse responses [98]. Also the noise power of the channel was obtained as [15]:

$$P_n(f, d) = \int_B N(f, d)df = k_B \int_B T_{noise}(f, d)df \quad (1)$$

$$\simeq k_B \int_B T_{mol}(f, d)df$$

where, $T_{mol} = T_o(1 - e^{-4\pi fd\kappa/c})$ is the equivalent noise temperature due to molecular absorption; k_B is the Boltzmann constant; T_o is the reference temperature.

The capacity of the channel was also studied to evaluate the potential of the EM paradigm. Four different power spectral densities (p.s.d) were studied by [15] *i.e.*, optimal p.s.d., flat p.s.d., the Gaussian pulse and the p.s.d. for the case of the transmission window at 350 GHz, which concluded that for the very short communication range, quite high transmission bit-rates can be supported, up to Terabits per second indicating the promising future of the application of the EM mechanism for nano-communication. In the next subsections the modeling of human tissues at these frequencies are presented both numerically and experimentally.

A. Numerical Modeling at Terahertz Frequencies

In this section a modeling of homogenous and layered model to investigate the wave propagation at THz band inside

human tissues. is presented *et al.* [99], [100], while comparing the results with theoretical model presented above.

1) *Homogeneous Model:* In [101], absorption path loss in tissues was calculated by setting up a simple model, shown in Fig. 9, using CST Microwave Studio [102]. As plane wave attenuates in lossy materials, hence absorption path loss was calculated by studying plane wave in tissues. In this study a tissue cube was modeled by dielectric cube as shown in the Fig. 9, since the tissue size ($7mm \times 7mm \times 7mm$) is comparable to THz wavelength. Tab. II shows the permittivity of the human tissues used in this study, which are calculated from the optical parameters given in [14], [13]. The variation of E-field for a plane wave propagating in +z direction is monitored by equally spaced probes, while considering a perfect matched layer boundary condition. The comparison of analytically and numerically calculated absorption path loss (as shown in Fig. 10) validates the numerical model accuracy, thus paving a way forward for more studies.

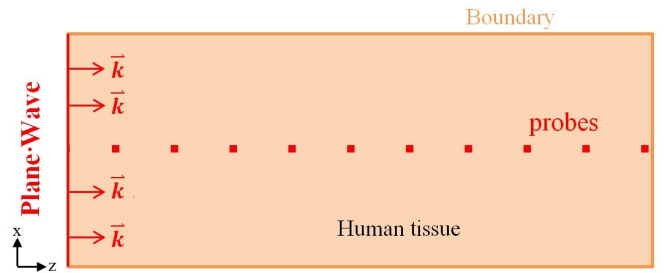


Fig. 9: A human tissue model for plane wave propagation [99].

TABLE II: The dielectric parameters at 1THz [99]

Tissues	Blood	Skin	Fat
ϵ'	3.5781	2.9240	2.2130
ϵ''	2.0109	0.9085	0.5732

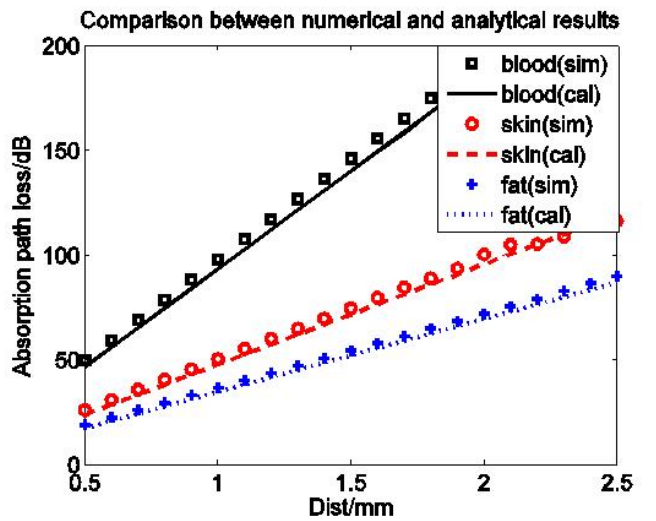


Fig. 10: Comparison of numerical and theoretical absorption pathloss at 1 THz [99]

2) *Layered Model*: In addition to simple model mentioned above, studies were also performed numerically in CST on layered structures as well (Fig. 11) by authors of this paper. A three layered model with the thickness of 1.5 mm (skin), 5 mm (fat) and 1.9 mm (muscle) was developed with perfectly matched layer boundary condition. Two dipoles were used in this simulation, where one was in skin and the other one was in fat. Two different scenarios *i.e.*, vertical and horizontal orientation of dipoles was considered. The comparison of power loss showed the minimum effect of the layered structure.

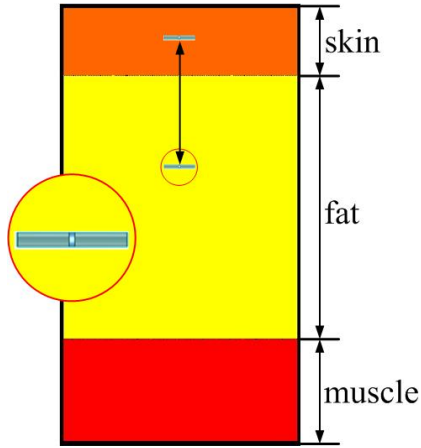


Fig. 11: A planar three layered human model at terahertz frequencies [99]

B. Measurement Techniques at Terahertz frequencies

The studies on the EM/Optical parameters of human tissues are quite limited in the THz band of interest [13], [14], [103]. Initially, pulsed base THz time domain spectroscopy (THz-TDS) was used to measure the absorbance of DNA, at the band of 0.06 to 2.0 THz [104]. Later, power absorption and far-infrared signal transmission at THz band inside animal tissues were measured using THz-TDS in [105]. Because the performance of the cancer is different from the healthy tissue at THz band, more and more studies are conducted on the characterisation of the human tissues at these bands.

Recently, spectroscopy measurements of normal and cancer breast tissue in the range 0.1 to 4 THz were conducted by Tyler Bowman and *et. al.* [106], demonstrating the potential of THz spectroscopy for the recognition of the cancer cell. However, most of the researches are still restricted to KHz or GHz of range [107], [108] because the biological material in this range is believed to have little scattering and the study of the tissue parameters at THz band is still in its early phase. In [14], [13], authors show the importance of THz pulse imaging system for characterizing biological tissues such as skin, muscle and veins. The work done in these papers was preliminary while considering very simple model. The authors did not consider skin type, specific layer and complexity of the tissue in their studies. It should be noted that freshly excised tissue are expected to have high water content but the comparison of dehydrated skin is missing in these references. The only plot

to account for skin behavior is absorption coefficient, which is indeed high for a fresh tissue.

To enrich the database of the parameters for biological tissues at THz band, the human tissue samples obtained from Blizzard Institute are measured with the THz-TDS system (shown in Fig. 12) at Queen Mary University of London [109], [110]. A novel channel model was presented by Abbasi *et al.* in [109] (authors of this paper) as a parameter of frequency, distance and sweat ducts. Results are validated by THz-TDS measurements of real skin with reasonably good agreement as shown in Fig. 14. The THz-TDS measurements of artificial skin (collagen) (Fig. 13), the main constitute of epidermis was performed in [110], to investigate if it is enough to use the parameters of collagen as the epidermis at the band of interest by studying both dielectric constants and channel parameters.

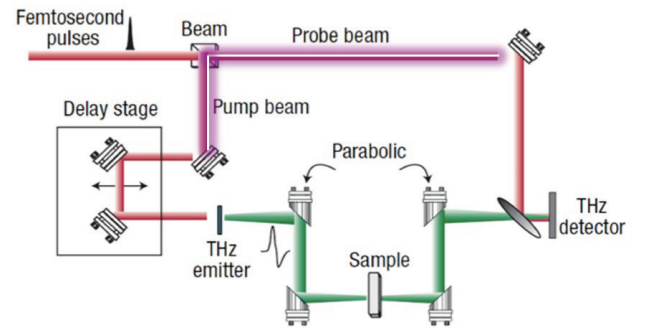


Fig. 12: Terahertz Time Domain Spectroscopy measurement setup at Queen Mary University of London [110].

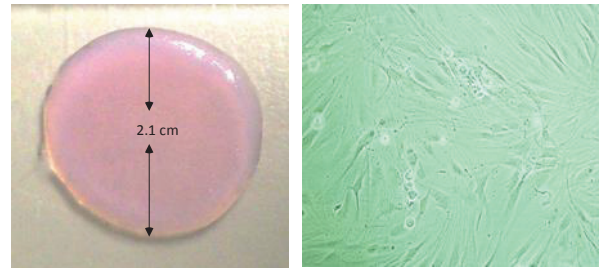


Fig. 13: Artificial Skin (collagen) cultured in the Blizzard Institute, QMUL (left) & Collagen layer growth by fibroblast cells (right) [110].

VII. NETWORK AND SYSTEM MODELS

Due to the very high path-loss introduced by the intra-body channel (Sec. VI) and in light of the very limited power of nano-devices (Sec. V), nanonetworks or networks of nano-devices will be needed to realize many of the aforementioned applications (Sec. II). In this section, the state of the art and open challenges at the network or system level are presented. Traditional TCP/IP protocol stack model is not feasible for implementation in nanonetworks since the TCP/IP model was originally designed for the high processing of general purpose

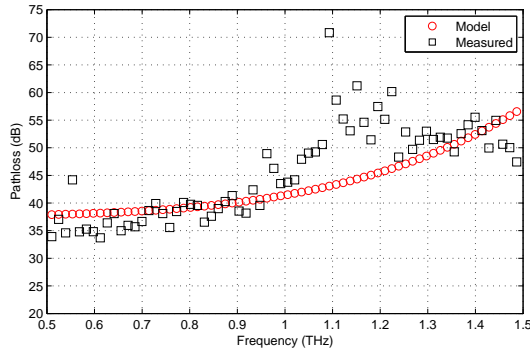


Fig. 14: Comparison of measured (THz TDS) and modeled path loss inside the skin at THz frequencies [109].

network nodes. Conversely, nanomachines nodes are limited in power supply, processing, and communication range due to high pathloss as mentioned above. Currently, introducing an innovative protocol stack model that captures the specific characteristics of nanonetworks is still in its early stages and an active area of research. Several proposals in current literature address the nanonetworks protocol stack as the proposals can be categorized into two main categories: No-layer models and Layer-based models, and .

A. No-Layer-Based Models

Layer-based protocol stack assumes that nanonetworks maintain a multi-tiered, dynamic, and opportunistic hierarchical architecture that comprise nanomachines, nano-router, and gateway. Nanomachines can be further clustered so that each group that serves a certain body area or a certain purpose is managed by a cluster head that will handle data propagation to the nano-router [6]. The hierarchy tree from nanomachines to back-end servers needs to be dynamic; connectivity from nanomachines to cluster heads and from cluster heads to gateways can change according to context and availability. Thus, nano-routers can opportunistically connect to the nearest gateway in order to send data. Nano-routers and cluster heads are assumed to have relatively higher processing power and larger bulks. Sizeable nano-routers may not feasibly reside within nanonetworks for some applications or environments under monitoring due to several factors, such as the environment structure, scalability and placement issues. Hence, these concerns can be addressed by assuming one-tiered nanonetworks, which consider identical network nodes with low processing and power capabilities, and simplified networking models. Specifically, no-layer-based models enforced by the limitations of the nanomachine nodes motivate the single layer paradigms, where the function of the Datalink, Network, Transport, and Application layer is combined in the Physical layer mainly through signal flooding communication. Signal flooding abolishes the requirements for node addressing, identification, routing and forwarding schemes. The work in [111] proposed a no-layer-based networking paradigm and flooding data dissemination scheme. The proposed scheme, though simplifying the communication model, overlooks the

cost of classification and real time signal processing of each packet. Additionally, it assumes fixed structure and static node deployment. The nanonodes typically display random behavior. Nanonetworks can move around the human body for certain health applications, and therefore may need to be associated with different neighbors and thus may not always acquire fixed structure. Comparatively, nanonetworks deployed for environment monitoring may get affected by wind movement, which will affect their location, and therefore may associate with different neighbors along their path.

B. Layer-Based Models

Some proposals attempted to implement a minor form of TCP/IP model regardless of the constraints of the employment of TCP/IP model in nanonetworks, while other proposals suggested the use of layer-based models specifically designed for nanonetworks. In the next section, a networking layer-based technique is presented, by following a bottom-up approach.

1) Link Layer:

- *Synchronization*: The transmission of low-power signals at very high frequencies, and potentially using very high data-rates, leads to many synchronization challenges. Tight synchronization between the transmitter and the receiver is needed to guarantee the proper detection of individual symbols. Unfortunately, we cannot simply reuse existing solutions for high-frequency communication schemes, such as Impulse Radio Ultra-wide-band (IR-UWB), Millimeter Wave (mm-wave) or Free Space Optical (FSO) systems, mainly because these rely on the use of high-speed Analog-to-Digital (ADCs). The fastest existing ADC to date can only sample at rates below 100 Giga-Samples-per-second (GSas) [112], much below the Nyquist rate for THz signals. Furthermore, its size and power consumption make it inadequate for nano-devices. In addition to the lack of ADCs, the local clock [113] at different nano-devices might oscillate at slightly different frequencies, which can result in a significant clock skew between the transmitter and the receiver.

To overcome these limitations, new time and frequency synchronization algorithms are needed. One the one hand, fully analog synchronization schemes can be developed to overcome the need for faster and smaller ADCs. For example, in [114], a synchronization scheme for pulse-based THz-band communications is designed and analyzed. The proposed scheme is aimed at iteratively estimating the symbol start time and reducing the observation window length for the symbol detector, and it can be implemented with a combination of voltage-controlled delay (VCD) lines [115] and Continuous-Time Moving-Average (CTMA) symbol detectors [116]. Another option could be to take advantage of sub-Nyquist sampling strategies, which could then be implemented with existing low-power slower ADCs. For example, in [117], a low-sampling-rate (LSR) synchronization algorithm is developed, by extending the theory of sampling signals with finite rate of innovation in the communication context and exploiting the annihilating filter method.

- *Error Control:* The combination of low transmission power, molecular absorption noise and multi-user interference in nanonetworks lead to error-prone wireless links. Traditional error control schemes, such as Automatic Repeat reQuest (ARQ) or Forward Error Correction (FEC) techniques, need to be analyzed in light of the peculiarities of nanonetworks. For example, on the one hand, Automatic Repeat reQuest (ARQ) mechanisms might not be suited for nanonetworks due to the energy limitations of nano-devices, which require nanoscale energy harvesting mechanisms to operate [118], [119]. The very long time needed to harvest enough energy to retransmit a packet make render the data useless. On the other hand, the majority of Forward Error Correction (FEC) mechanisms are just too complex for the expected capabilities of the nano-devices. As described in [5], the number of nano-transistors in a nano-processor limits the complexity of the operations that it can complete. Even with current processing technologies, the time needed to encode and decode a packet can be much longer than the packet transmission time.

To overcome these limitations, new error control strategies are needed. On the one hand, much simpler coding schemes tailored both to the capabilities of nano-devices and the peculiarities of the THz-band channel can be developed. In this direction, the use of low-weight Error Prevention Codes (EPCs) has been proposed [120]. More specifically, it has been shown that the reduction of the average number of logic ones transmitted per packet results in a decrease in the overall molecular-absorption noise and interference powers. However, the reduction of the coding weight requires the transmission of longer data packets, which results in a higher energy consumption both at the transmitter and the receiver when compared to that of uncoded transmission [121]–[123]. For this, on the other hand, there is a need for a unified cross-layer error-control analysis, tailored to the peculiarities of nanonetworks both on the nano-device side and the communication side. For example, in [124], a mathematical framework is developed and used to analyze the tradeoffs between Bit Error Rate (BER), Packet Error Rate (PER), energy consumption and latency, for different error-control strategies, namely, ARQ, FEC, EPC and a hybrid EPC.

- *Medium Access Control:* New Medium Access Control (MAC) protocols are needed to regulate the channel access in nanonetworks. In traditional wireless communication networks, the main bottleneck at the link layer is posed by the limited available bandwidth, which forces nodes to either aggressively contend for the channel or follow tight time scheduling schemes. In nanonetworks, the THz-band channel provides nano-devices with a huge bandwidth and relaxes the need to “fight” or wait for the channel. In addition, such very large bandwidth results in very high bit-rates and, consequently, very short transmission times, which further minimize the collision probability. However, the low transmission power of THz nano-transceivers, the high path-loss at THz-band

frequencies and the limited and fluctuating energy of nano-devices, still require the use of MAC protocols to regulate the link behavior.

In this direction, several new protocols have been recently proposed. In [67], the Physical-layer Aware MAC Protocol for Electromagnetic Nanonetworks (PHLAME) was proposed, effectively becoming the first MAC protocol for ad-hoc nanonetworks. In this protocol, nano-devices are able to dynamically choose different physical layer parameters based on the channel conditions and the energy of the nano-devices. Similarly, in [125], the first centralized MAC protocol for nanonetworks was proposed, in which a nano-controller would determine the best communication parameters for the nano-devices. In both cases, a transmitter-initiated hand-shake was required, which would eventually result into a low channel utilization. In [126], a receiver-initiated MAC protocol for nanosensor networks was proposed. The developed protocol is based on a distributed scheduling scheme, which requires the nodes to perform a distributed edge coloring algorithm. However, due to the very limited computational resources of individual nano-devices, it seems more plausible to leverage the pulse-based physical layer to interleave users in time, rather than performing distributed scheduling algorithms. More recently, in [127], a joint link-layer synchronization and MAC protocol for THz communication networks has been presented. The protocol relies on a receiver-initiated handshake as a way to guarantee synchronization between transmitter and receiver. In addition, it incorporates a sliding window flow control mechanism, which combined with the one-way handshake, maximizes the channel utilization.

C. Network and Transport Layers

- *Relaying:* At THz-band frequencies, the very large available bandwidth comes at the cost of a much higher path-loss than that of lower frequency bands. Because of the very limited transmission power of nano-devices, this results into very short transmission distances (much below one meter). However, in the aforementioned applications, very large node densities are needed and, thus, intensive relaying is expected. Traditional analysis of optimal relaying studies [128], [129] are not applicable to nanonetworks, because they do not take into account the peculiarities of the THz-band channel. At THz-band frequencies, the benefit of relaying is twofold. As in any wireless communication system, the transmission power and, thus, the energy consumption can be reduced by having several intermediate hops between the transmitter and the receiver. In addition, due to the unique distance-dependent behavior of the bandwidth in the THz band, the reduction of the transmission distance results into the availability of a wider transmission band because fewer absorbing molecules are found along the path. Larger bandwidths result in faster data rates and, thus, can help to further reduce the energy-per-bit consumption, the packet transmission time, and the collision probability. However,

by increasing the number of hops, the overhead in the network increases. All these motivate the development of new relaying strategies, which take into account both the possibility to utilize active nodes as well as novel passive relaying nodes based on dielectric mirrors [130].

- *Routing*: New routing protocols for multi-hop communication in nanonetworks need to be developed by taking into account the nano-device capabilities and the behavior of the the lower layers in the protocol stack. Routing information across multiple links with unknown relaying nano-nodes is a non-trivial task. First, as just discussed, the distance and actual molecular composition of the channel needs to be taken into account when making routing decisions. Taking the channel conditions into account at the routing metric is not new, but rather common in cross-layer routing solutions. The difference in this case is the origin of such channel change, i.e., molecular absorption, which results in higher energy consumption and longer transmission delays. In this direction, in [131], a new routing framework was developed, based on three main tasks, namely, the evaluation of the probability of saving energy through a multi-hop transmission, the tuning of the transmission power of each nanosensor for throughput and hop distance optimization, and the selection of the next hop nanosensor on the basis of their available energy and current load. Still, however, an additional challenge comes from the very limited computational resources of nano-devices. This requires the development of novel strategies different from the traditional “store and forward” protocols. For example, as in Networks-on-Chip (NoC) [132], [133] or optical core networks [134], [135], it might not be worth to “wait” until identifying the best route for a packet, but rather keep forwarding it even if it might not follow the optimal path to the destination.
- *Reliable Transport*: Last but not least, the interconnection of intra-body nanomachines with wearable devices and ultimately the Internet will require the development of end-to-end solutions that can guarantee the reliable transport. On the one hand, new extensions to the Transport Control Protocol (TCP) protocol need to be developed. It is a fact that the majority of traffic over the Internet is transported by TCP. Therefore, it seems reasonable to modify and improve the performance of TCP while keeping backwards compatibility, rather than directly proposing radically new protocols. New algorithms to control the behavior of the congestion window size in TCP are needed, which take into account the huge available bandwidth in the THz-band and the near-zero memory of the nano-devices along the path. These could be estimated in a cross-layer fashion, following a similar approach as in ultra-high-speed wired optical communication networks [136]. On the other hand, in the applications in which the use of classical transport layer solutions is not required, fundamentally different protocols can be developed. In nanonetworks, robust transport layer solutions are necessary to deal with frequent device failures, disconnections due to energy fluctuations, or molecular

channel composition transient effects. All these motivate also the development of cross-layer solutions [137], which can jointly capture the device, communication and networking peculiarities.

VIII. OPEN RESEARCH CHALLENGES

With the growing interest in nano-technology especially in biomedical domain and their advantage to provide substantial flexibility and improvement in healthcare for diagnostics and treatment of more diseases will likely increase their usage in time. Some of the most important open research topics in this domain are given as follows:

- *Human tissue parameters extraction at terahertz frequencies*: Although some optical parameters are provided at such frequencies but the study of the tissue parameters at THz band is still in its infancy. Hence a through database of tissue properties is needed at such frequencies based on the large number of samples to better understand and model the electromagnetic wave behavior inside these materials, which is very important for developing efficient and accurate nano based health system.
- *Safety constraints, Heating problems at THz frequencies*: Safety issue is always the main consideration about nano-network, especially when the nano-devices are applied to the in-body scenario. Hence, the study of the THz wave heating effects on the human tissue should be conducted to make the standard and requirement for communicating or sensing.
- *Interaction between the nano-devices and the surrounding environment*: From the study of the models of nerve system and skin, it seems dispensable to study the detailed model when the size of the functional devices goes down to milli/nano-scale. The interaction between the environment and the devices should be study to make sure the devices work in a desired manner.
- *Hybrid nano-communication systems*: Since there are lots of communication paradigms for nano-communication, the study on interaction between two different communications paradigm is still missing. It is generally believed that by merging all the communications together the nano-network would be much more flexible and powerful. Hence studies on hybrid communication mechanism and their feasibility is much needed future direction.
- *Architecture and protocols*: Different challenges against protocols design are still being investigated with no currently fully developed solutions. Currently, introducing an innovative protocol stack model that captures the specific characteristics of nanonetworks is still in its early stages and an active area of research.
- *Antenna design and propagation models*: In order to support high data rates and overcome very high pathloss at such frequencies a compact large antenna array with multi-band and ultra-broadband characteristics is needed. Also, in such networks, molecular noise, nano-particle scattering and multipath fading are additional parameters on top of high pathloss, which effect signal propagation. Hence an accurate channel model, taking into account

all propagation effects still need to be developed, which are very important for accurate link budget calculation needed to develop highly efficient and reliable systems.

- *Massive MIMO and cooperative communication*: To overcome the high pathloss issues and other propagation hurdles like scattering and multipath fading, massive MIMO and cooperative communication based methods are very promising. However, the knowledge of spatial correlation inside the body medium should be investigated for facilitating the implementation of these techniques and understanding the maximum achievable channel capacity.
- *Security*: Security of health related information is very critical and ensuring the secure transmission especially between nano- and micro-device interface and gateway is very crucial. Therefore, robust, security (including authentication and privacy) ensuring algorithms are essential for confidently using these devices.
- *Nano sensor integration*: Several nano-devices are developed and tested under strict laboratory condition, but integrating all nano components including sensor, battery, memory *etc* is still an open challenge, which needs great attention.

IX. CONCLUSION

In this paper, the state-of-the-art and comprehensive review in the domain of nano-scale electromagnetic communication specifically for biomedical applications is presented. Various studies have been analysed and discussed covering the theoretical basis of communication mechanisms among nano devices, state-of-the-art in antenna design, human tissue and the channel modeling based on numerical and experimental settings. In addition, we highlighted in the paper the current state of network and system modeling specifically aimed at nano-scale communications and linked those to future directions and needed research solutions to overcome current challenges. Considering the expected future growth of nano technologies and their potential use for the detection and diagnosis of various health related issues, the open research challenges for these potential networks (in the medium to long term) are highlighted and presented to clearly demonstrate the necessary steps the scientific, engineering and wider community needs to take to further enhance the current status and ensure applicability not only in the biomedical domain but a broader range of deployments.

ACKNOWLEDGMENT

This publication was made possible by NPRP grant # 7-125-2-061 from the Qatar National Research Fund (a member of Qatar Foundation). The statements made herein are solely the responsibility of the authors.

REFERENCES

- [1] Metin Sitti, Hakan Ceylan, Wenqi Hu, Joshua Giltinan, Mehmet Turan, Sehyuk Yim, and Eric Diller. Biomedical applications of untethered mobile milli/microrobots. *Proceedings of the IEEE*, 103(2):205–224, 2015.
- [2] Ian F Akyildiz, Fernando Brunetti, and Cristina Blázquez. Nanonetworks: A new communication paradigm. *Computer Networks*, 52(12):2260–2279, 2008.
- [3] Sasitharan Balasubramanian and Jussi Kangasharju. Realizing the internet of nano things: challenges, solutions, and applications. *Computer*, (2):62–68, 2013.
- [4] Giuseppe Piro, Ke Yang, Gennaro Boggia, Nishtha Chopra, Luigi Grieco, and Akram Alomainy. Terahertz communications in human tissues at the nano-scale for healthcare applications. *Nanotechnology, IEEE Transactions on*, 2015.
- [5] I. F. Akyildiz and J. M. Jornet. Electromagnetic wireless nanosensor networks. *Nano Communication Networks (Elsevier) Journal*, 1(1):3–19, March 2010.
- [6] I. F. Akyildiz and J. M. Jornet. The internet of nano-things. *IEEE Wireless Communications Magazine*, 17(6):58–63, December 2010.
- [7] Serge Luryi, Jimmy Xu, and Alexander Zaslavsky. *Future Trends in Microelectronics: Frontiers and Innovations*. John Wiley & Sons, 2013.
- [8] Peter S. Hall and Yang Hao. *Antennas and Propagation for Body-Centric Wireless Communication*. Artech House, 2012.
- [9] Qammer Hussain Abbasi, Andrea Sani, Akram Alomainy, and Yang Hao. Numerical characterization and modeling of subject-specific ultrawideband body-centric radio channels and systems for healthcare applications. *Information Technology in Biomedicine, IEEE Transactions on*, 16(2):221–227, 2012.
- [10] T. Binzoni, A. Vogel, A. H. Gandjbakhche, and R. Marchesini. Detection limits of multi-spectral optical imaging under the skin surface. *Physics in medicine and biology*, 53:617–636, 2008.
- [11] Cecil S Joseph, Anna N Yaroslavsky, Victor A Neel, Thomas M Goyette, and Robert H Giles. Continuous wave terahertz transmission imaging of nonmelanoma skin cancers. *Lasers in Surgery and Medicine*, 43(6):457–462, 2011.
- [12] Euna Jung, Hongkyu Park, Kiwon Moon, Meehyun Lim, Youngwoong Do, Haewook Han, Hyuck Jae Choi, Byung-Hyun Min, Sangin Kim, Ikmo Park, et al. Thz time-domain spectroscopic imaging of human articular cartilage. *Journal of Infrared, Millimeter, and Terahertz Waves*, 33(6):593–598, 2012.
- [13] Elizabeth Berry, Anthony J Fitzgerald, Nickolay N Zinov’ev, Gillian C Walker, Shervanthi Homer-Vanniasinkam, Caroline D Sudworth, Robert E Miles, J Martyn Chamberlain, and Michael A Smith. Optical properties of tissue measured using terahertz-pulsed imaging. In *Medical Imaging 2003*, pages 459–470. International Society for Optics and Photonics, 2003.
- [14] AJ Fitzgerald, E Berry, NN Zinov’ev, S Homer-Vanniasinkam, RE Miles, JM Chamberlain, and MA Smith. Catalogue of human tissue optical properties at terahertz frequencies. *Journal of Biological Physics*, 29(2-3):123–128, 2003.
- [15] J. M. Jornet and I. F. Akyildiz. Channel modeling and capacity analysis of electromagnetic wireless nanonetworks in the terahertz band. *IEEE Transactions on Wireless Communications*, 10(10):3211–3221, October 2011.
- [16] Gerald J Wilmink and Jessica E Grundt. Invited review article: current state of research on biological effects of terahertz radiation. *Journal of Infrared, Millimeter, and Terahertz Waves*, 32(10):1074–1122, 2011.
- [17] G Enrico Santagati and Tommaso Melodia. Opto-ultrasonic communications for wireless intra-body nanonetworks. *Nano Communication Networks*, 5(1):3–14, 2014.
- [18] Robert A Freitas. Nanotechnology, nanomedicine and nanosurgery. *International Journal of Surgery*, 3(4):243–246, 2005.
- [19] Zhuan Liao, Rui Gao, Can Xu, and Zhao-Shen Li. Indications and detection, completion, and retention rates of small-bowel capsule endoscopy: a systematic review. *Gastrointestinal endoscopy*, 71(2):280–286, 2010.
- [20] Tetsuya Nakamura and Akira Terano. Capsule endoscopy: past, present, and future. *Journal of gastroenterology*, 43(2):93–99, 2008.
- [21] Guobing Pan and Litong Wang. Swallowable wireless capsule endoscopy: Progress and technical challenges. *Gastroenterology research and practice*, 2012, 2011.
- [22] M Fluckiger and Bradley J Nelson. Ultrasound emitter localization in heterogeneous media. In *Engineering in Medicine and Biology Society, 2007. EMBS 2007. 29th Annual International Conference of the IEEE*, pages 2867–2870. IEEE, 2007.
- [23] Kang Kim, Laura A Johnson, Congxian Jia, Joel C Joyce, Sujal Rangwalla, Peter DR Higgins, and Jonathan M Rubin. Noninvasive ultrasound elasticity imaging (uei) of crohn’s disease: animal model. *Ultrasound in medicine & biology*, 34(6):902–912, 2008.
- [24] Olgaç Ergeneman, Gökem Dogangil, Michael P Kummer, Jake J Abbott, Mohammad K Nazeeruddin, and Bradley J Nelson. A magnetically controlled wireless optical oxygen sensor for intraocular measurements. *Sensors Journal, IEEE*, 8(1):29–37, 2008.

- [25] J Matthew Dubach, Daniel I Harjes, and Heather A Clark. Fluorescent ion-selective nanosensors for intracellular analysis with improved lifetime and size. *Nano Letters*, 7(6):1827–1831, 2007.
- [26] Jianping Li, Tuzhi Peng, and Yuqiang Peng. A cholesterol biosensor based on entrapment of cholesterol oxidase in a silicic sol-gel matrix at a prussian blue modified electrode. *Electroanalysis*, 15(12):1031–1037, 2003.
- [27] Padmavathy Tallury, Astha Malhotra, Logan M Byrne, and Swadeshmukul Santra. Nanobioimaging and sensing of infectious diseases. *Advanced drug delivery reviews*, 62(4):424–437, 2010.
- [28] Jonathan W Aylott. Optical nanosensors enabling technology for intracellular measurements. *Analyst*, 128(4):309–312, 2003.
- [29] Ph Avouris, G Dresselhaus, and MS Dresselhaus. Carbon nanotubes: synthesis, structure, properties and applications. *Topics in Applied Physics*, 2000.
- [30] S Tasoglu, E Diller, S Guven, M Sitti, and U Demirci. Untethered micro-robotic coding of three-dimensional material composition. *Nature communications*, 5, 2014.
- [31] Ira J Fox, George Q Daley, Steven A Goldman, Johnny Huard, Timothy J Kamp, and Massimo Trucco. Use of differentiated pluripotent stem cells as replacement therapy for treating disease. *Science*, 345(6199):1247391, 2014.
- [32] Sangwon Kim, Famin Qiu, Samhwan Kim, Ali Ghanbari, Cheil Moon, Li Zhang, Bradley J Nelson, and Hongsoo Choi. Fabrication and characterization of magnetic microrobots for three-dimensional cell culture and targeted transportation. *Advanced Materials*, 25(41):5863–5868, 2013.
- [33] K Eric Drexler. *Nanosystems: molecular machinery, manufacturing, and computation*. John Wiley & Sons, Inc., 1992.
- [34] Robert A Freitas. What is nanomedicine? *Nanomedicine: Nanotechnology, Biology and Medicine*, 1(1):2–9, 2005.
- [35] Rodrigo Fernández-Pacheco, Clara Marquina, J Gabriel Valdivia, Martín Gutiérrez, M Soledad Romero, Rosa Cornudella, Alicia Laborda, Américo Vilorio, Teresa Higuera, Alba García, et al. Magnetic nanoparticles for local drug delivery using magnetic implants. *Journal of Magnetism and Magnetic Materials*, 311(1):318–322, 2007.
- [36] Robert A Freitas. Pharmacocytes: An ideal vehicle for targeted drug delivery. *Journal of Nanoscience and Nanotechnology*, 6(9-10):2769–2775, 2006.
- [37] Brian P Timko, Tal Dvir, and Daniel S Kohane. Remotely triggerable drug delivery systems. *Advanced materials*, 22(44):4925–4943, 2010.
- [38] Sehyuk Yim and Metin Sitti. Shape-programmable soft capsule robots for semi-implantable drug delivery. *Robotics, IEEE Transactions on*, 28(5):1198–1202, 2012.
- [39] Rika Wright Carlsen and Metin Sitti. Bio-hybrid cell-based actuators for microsystems. *Small*, 10(19):3831–3851, 2014.
- [40] Ching-Jen Chen, Drs Yousef Haik, and Jhunu Chatterjee. Development of nanotechnology for biomedical applications. In *Emerging Information Technology Conference, 2005.*, pages 4–pp. IEEE, 2005.
- [41] Edward B Steager, Mahmut Selman Sakar, Ceridwen Magee, Monroe Kennedy, Anthony Cowley, and Vijay Kumar. Automated biomanipulation of single cells using magnetic microrobots. *The International Journal of Robotics Research*, 32(3):346–359, 2013.
- [42] Tomohiro Kawahara, Masakuni Sugita, Masaya Hagiwara, Fumihito Arai, Hiroyuki Kawano, Ikuko Shihira-Ishikawa, and Atsushi Miyawaki. On-chip microrobot for investigating the response of aquatic microorganisms to mechanical stimulation. *Lab on a Chip*, 13(6):1070–1078, 2013.
- [43] Deok-Ho Kim, Pak Kin Wong, Jungyul Park, Andre Levchenko, and Yu Sun. Microengineered platforms for cell mechanobiology. *Annual review of biomedical engineering*, 11:203–233, 2009.
- [44] Kyoung-Chul Kong, Jinhoon Cha, Doyoung Jeon, and Dong-il Dan Cho. A rotational micro biopsy device for the capsule endoscope. In *Intelligent Robots and Systems, 2005.(IROS 2005). 2005 IEEE/RSJ International Conference on*, pages 1839–1843. IEEE, 2005.
- [45] Piero Miloro, Edoardo Sinibaldi, Arianna Menciaci, and Paolo Dario. Removing vascular obstructions: a challenge, yet an opportunity for interventional microdevices. *Biomedical microdevices*, 14(3):511–532, 2012.
- [46] Sehyuk Yim, Evin Gultepe, David H Gracias, and Metin Sitti. Biopsy using a magnetic capsule endoscope carrying, releasing, and retrieving untethered microgrippers. *Biomedical Engineering, IEEE Transactions on*, 61(2):513–521, 2014.
- [47] Martin Heil and Jurriaan Ton. Long-distance signalling in plant defence. *Trends in plant science*, 13(6):264–272, 2008.
- [48] Corne MJ Pieterse and Marcel Dicke. Plant interactions with microbes and insects: from molecular mechanisms to ecology. *Trends in plant science*, 12(12):564–569, 2007.
- [49] Jongyoon Han, Jianping Fu, and Reto B Schoch. Molecular sieving using nanofilters: past, present and future. *Lab on a Chip*, 8(1):23–33, 2008.
- [50] Alex M Andrew. Nanomedicine, volume 1: Basic capabilities. *Kybernetes*, 29(9/10):1333–1340, 2000.
- [51] M. Pierobon and I.F. Akyildiz. A Physical End-to-End Model for Molecular Communication in Nanonetworks. *IEEE J. Sel. Areas Commun.*, 28(4):602–611, May 2010.
- [52] Mehmet kr Kuran, H. Birkan Yilmaz, Tuna Tugcu, and Bilge zerman. Energy Model for Communication via Diffusion in Nanonetworks. *J. Nano Commun. Networks*, 1(2):86 – 95, 2010.
- [53] M. Pierobon and I.F. Akyildiz. Diffusion-Based Noise Analysis for Molecular Communication in Nanonetworks. *IEEE Trans. Signal Process.*, 59(6):2532–2547, June 2011.
- [54] Po-Jen Shih, Chia-Han Lee, Ping-Cheng Yeh, and Kwang-Cheng Chen. Channel Codes for Reliability Enhancement in Molecular Communication. *IEEE J. Sel. Areas Commun.*, 31(12):857–867, December 2013.
- [55] A. Einolghozati, M. Sardari, and F. Fekri. Relaying in Diffusion-based Molecular Communication. In *IEEE International Symposium on Information Theory (ISIT)*, pages 1844–1848, July 2013.
- [56] T. Nakano and Jian-Qin Liu. Design and Analysis of Molecular Relay Channels: An Information Theoretic Approach. *IEEE Trans. NanoBioscience*, 9(3):213–221, Sept 2010.
- [57] Yuanfeng Chen, Panagiotis Kosmas, Putri Anwar, and Liwen Huang. A touch-communication framework for drug delivery based on a transient microbot system. *Nanobioscience, IEEE Transactions on*, 14(4):397–408, 2015.
- [58] I.S.M. Khalil, V. Magdanz, S. Sanchez, O.G. Schmidt, L. Abelmann, and S. Misra. Magnetic control of potential microrobotic drug delivery systems: Nanoparticles, magnetotactic bacteria and self-propelled microjets. In *Engineering in Medicine and Biology Society (EMBC), 2013 35th Annual International Conference of the IEEE*, pages 5299–5302, July 2013.
- [59] Tad Hogg and Robert A Freitas Jr. Acoustic communication for medical nanorobots. *Nano Communication Networks*, 3(2):83–102, 2012.
- [60] G Enrico Santagati and Tommaso Melodia. Opto-ultrasonic communications in wireless body area nanonetworks. In *Signals, Systems and Computers, 2013 Asilomar Conference on*, pages 1066–1070. IEEE, 2013.
- [61] Suk-Won Hwang, Hu Tao, Dae-Hyeong Kim, Huanyu Cheng, Jun-Kyul Song, Elliott Rill, Mark A Brenckle, Bruce Panilaitis, Sang Min Won, Yun-Soung Kim, et al. A physically transient form of silicon electronics. *Science*, 337(6102):1640–1644, 2012.
- [62] Sylvain Martel, Mahmood Mohammadi, Ouajdi Felfoul, Zhao Lu, and Pierre Pouponneau. Flagellated magnetotactic bacteria as controlled mri-trackable propulsion and steering systems for medical nanorobots operating in the human microvasculature. *The International journal of robotics research*, 28(4):571–582, 2009.
- [63] Sylvain Martel, Ouajdi Felfoul, Jean-Baptiste Mathieu, Arnaud Chanu, Samer Tamaz, Mahmood Mohammadi, Martin Mankiewicz, and Nasr Tabatabaei. Mri-based medical nanorobotic platform for the control of magnetic nanoparticles and flagellated bacteria for target interventions in human capillaries. *The International journal of robotics research*, 28(9):1169–1182, 2009.
- [64] Yifan Chen, Panagiotis Kosmas, and Rui Wang. Conceptual design and simulations of a nano-communication model for drug delivery based on a transient microbot system. In *Antennas and Propagation (EuCAP), 2014 8th European Conference on*, pages 63–67. IEEE, 2014.
- [65] M Rosenau da Costa, OV Kibis, and ME Portnoi. Carbon nanotubes as a basis for terahertz emitters and detectors. *Microelectronics Journal*, 40(4):776–778, 2009.
- [66] C Emre Koksal and Eylem Ekici. A nanoradio architecture for interacting nanonetworking tasks. *Nano Communication Networks*, 1(1):63–75, 2010.
- [67] J. M. Jornet, Joan Capdevila-Pujol, and Josep Sole-Pareta. Phlame: A physical layer aware mac protocol for electromagnetic nanonetworks in the terahertz band. *Nano Communication Networks (Elsevier) Journal*, 3(1):74 – 81, 2012.
- [68] Mona Nafari and Josep Miquel Jornet. Metallic plasmonic nano-antenna for wireless optical communication in intra-body nanonetworks. In *in Proc. of 10th EAI International Conference on Body Area Networks (BodyNets 2015), Sydney, Australia*, 2015.

- [69] Zhongkun Ma and Guy AE Vandenbosch. Systematic full-wave characterization of real-metal nano dipole antennas. *Antennas and Propagation, IEEE Transactions on*, 61(10):4990–4999, 2013.
- [70] Mario Bareiß, Badri N Tiwari, Andreas Hochmeister, Gunther Jegert, Ute Zschieschang, Hagen Klauk, Bernhard Fabel, Giuseppe Scarpa, Gregor Koblmüller, Gary H Bernstein, et al. Nano antenna array for terahertz detection. *Microwave Theory and Techniques, IEEE Transactions on*, 59(10):2751–2757, 2011.
- [71] Supriyo Datta. *Electronic transport in mesoscopic systems*. Cambridge university press, 1997.
- [72] Guanghui Zhou, Mou Yang, Xianbo Xiao, and Yuan Li. Electronic transport in a quantum wire under external terahertz electromagnetic irradiation. *Physical Review B*, 68(15):155309, 2003.
- [73] George W Hanson. Fundamental transmitting properties of carbon nanotube antennas. *Antennas and Propagation, IEEE Transactions on*, 53(11):3426–3435, 2005.
- [74] Peter J Burke, Shengdong Li, and Zhen Yu. Quantitative theory of nanowire and nanotube antenna performance. *Nanotechnology, IEEE Transactions on*, 5(4):314–334, 2006.
- [75] George W. Hanson. Dyadic Green’s functions and guided surface waves for a surface conductivity model of graphene. *Journal of Applied Physics*, 103(6):064302, 2008.
- [76] J. M. Jornet and I. F. Akyildiz. Graphene-based nano-antennas for electromagnetic nanocommunications in the terahertz band. In *Proc. of 4th European Conference on Antennas and Propagation, EUCAP*, April 2010.
- [77] Y-M Lin, Christos Dimitrakopoulos, Keith A Jenkins, Damon B Farmer, H-Y Chiu, Alfred Grill, and Ph Avouris. 100-ghz transistors from wafer-scale epitaxial graphene. *Science*, 327(5966):662–662, 2010.
- [78] Zheng Xu, Xiaodai Dong, and Jens Bornemann. Design of a reconfigurable mimo system for thz communications based on graphene antennas. *Terahertz Science and Technology, IEEE Transactions on*, 4(5):609–617, 2014.
- [79] Rajni Bala and Anupma Marwaha. Development of computational model for tunable characteristics of graphene based triangular patch antenna in thz regime. *Journal of Computational Electronics*, pages 1–6, 2015.
- [80] Rajni Bala and Anupma Marwaha. Investigation of graphene based miniaturized terahertz antenna for novel substrate materials. *Engineering Science and Technology, an International Journal*, 2015.
- [81] Jie Yang, Fanmin Kong, and Kang Li. Broad tunable nanoantenna based on graphene log-periodic toothed structure. *Plasmonics*, pages 1–6, 2015.
- [82] Josep Miquel Jornet and Ian F Akyildiz. Graphene-based plasmonic nano-antenna for terahertz band communication in nanonetworks. *Selected Areas in Communications, IEEE Journal on*, 31(12):685–694, 2013.
- [83] Jin Zhou, Tsung-Hao Chuang, Tolga Dinc, and Harish Krishnaswamy. 19.1 receiver with 20mhz bandwidth self-interference cancellation suitable for fdd, co-existence and full-duplex applications. In *Solid-State Circuits Conference-ISSCC, 2015 IEEE International*, pages 1–3. IEEE, 2015.
- [84] Multi-sensing ic for internet of things produced in taiwai.
- [85] David C Meeker, Eric H Maslen, Rogers C Ritter, and Francis M Creighton. Optimal realization of arbitrary forces in a magnetic stereotaxis system. *Magnetics, IEEE Transactions on*, 32(2):320–328, 1996.
- [86] K Ishiyama, M Sendoh, A Yamazaki, and KI Arai. Swimming micro-machine driven by magnetic torque. *Sensors and Actuators A: Physical*, 91(1):141–144, 2001.
- [87] J Yan, SA Avadhanula, J Birch, MH Dickinson, Metin Sitti, T Su, and RS Fearing. Wing transmission for a micromechanical flying insect. *Journal of Micromechatronics*, 1(3):221–237, 2001.
- [88] Seth Hollar, Anita Flynn, Colby Bellew, and KSJ Pister. Solar powered 10 mg silicon robot. In *Micro Electro Mechanical Systems, 2003. MEMS-03 Kyoto. IEEE The Sixteenth Annual International Conference on*, pages 706–711. IEEE, 2003.
- [89] Marco Quirini, Arianna Menciassi, Sergio Scapellato, Cesare Stefanini, and Paolo Dario. Design and fabrication of a motor legged capsule for the active exploration of the gastrointestinal tract. *Mechatronics, IEEE/ASME Transactions on*, 13(2):169–179, 2008.
- [90] Sehyuk Yim and Metin Sitti. Design and rolling locomotion of a magnetically actuated soft capsule endoscope. *Robotics, IEEE Transactions on*, 28(1):183–194, 2012.
- [91] Tian Qiu, Tung-Chun Lee, Andrew G Mark, Konstantin I Morozov, Raphael Münster, Otto Mierka, Stefan Turek, Alexander M Leshansky, and Peer Fischer. Swimming by reciprocal motion at low reynolds number. *Nature communications*, 5, 2014.
- [92] Caroline Cvetkovic, Ritu Raman, Vincent Chan, Brian J Williams, Madeline Tolish, Piyush Bajaj, Mahmut Selman Sakar, H Harry Asada, M Taher A Saif, and Rashid Bashir. Three-dimensionally printed biological machines powered by skeletal muscle. *Proceedings of the National Academy of Sciences*, 111(28):10125–10130, 2014.
- [93] Famin Qiu, Satoshi Fujita, Rami Mhanna, Li Zhang, Benjamin R Simona, and Bradley J Nelson. Magnetic helical microswimmers functionalized with lipoplexes for targeted gene delivery. *Advanced Functional Materials*, 25(11):1666–1671, 2015.
- [94] Chulwoo Son and Babak Ziaie. A wireless implantable passive microdosimeter for radiation oncology. *Biomedical Engineering, IEEE Transactions on*, 55(6):1772–1775, 2008.
- [95] Serge Luryi, Jimmy Xu, and Alex Zaslavsky. *Future trends in microelectronics: up the nano creek*. John Wiley & Sons, 2007.
- [96] Josep Miquel Jornet and Ian F Akyildiz. Channel capacity of electromagnetic nanonetworks in the terahertz band. In *Communications (ICC), 2010 IEEE International Conference on*, pages 1–6. IEEE, 2010.
- [97] C. Han, A. Bicen, and I. Akyildiz. Multi-ray channel modeling and wideband characterization for wireless communications in the terahertz band. *Wireless Communications, IEEE Transactions on*, PP(99):1–1, 2015.
- [98] J. Kokkonen, J. Lehtomaki, K. Umehayashi, and M. Juntti. Frequency and time domain channel models for nanonetworks in terahertz band. *Antennas and Propagation, IEEE Transactions on*, 63(2):678–691, Feb 2015.
- [99] Ke Yang, A. Pellegrini, M.O. Munoz, A. Brizzi, A. Alomainy, and Yang Hao. Numerical analysis and characterization of thz propagation channel for body-centric nano-communications. *Terahertz Science and Technology, IEEE Transactions on*, 5(3):419–426, May 2015.
- [100] K. Yang, Q.H. Abbasi, N. Chopra, M. Munoz, Y. Hao, and A. Alomainy. Effects of non-flat interfaces in human skin tissues on the In-Vivo THz communication channel. *Journal of Nano Communication Network*, Nov., 2015.
- [101] Ke Yang, Alessandro Pellegrini, Alessio Brizzi, Akram Alomainy, and Yang Hao. Numerical analysis of the communication channel path loss at the thz band inside the fat tissue. In *Microwave Workshop Series on RF and Wireless Technologies for Biomedical and Healthcare Applications (IMWS-BIO), 2013 IEEE MTT-S International*, pages 1–3. IEEE, 2013.
- [102] CST Microwave Studio. Cst microwave studio.
- [103] Dawn Lipscomb, Ibtissam Echchgadda, Xomalin G. Peralta, and Gerald J. Wilmsink. Determination of the optical properties of melanin-pigmented human skin equivalents using terahertz time-domain spectroscopy. volume 8585, 2013.
- [104] AG Markelz, A Roitberg, and EJ Heilweil. Pulsed terahertz spectroscopy of dna, bovine serum albumin and collagen between 0.1 and 2.0 thz. *Chemical Physics Letters*, 320(1):42–48, 2000.
- [105] Mingxia He, Abul K Azad, Shenghua Ye, and Weili Zhang. Far-infrared signature of animal tissues characterized by terahertz time-domain spectroscopy. *Optics Communications*, 259(1):389–392, 2006.
- [106] Tyler Bowman, Magda El-Shenawee, and Shubhra Gautam Sharma. Terahertz spectroscopy for the characterization of excised human breast tissue. In *Microwave Symposium (IMS), 2014 IEEE MTT-S International*, pages 1–4. IEEE, 2014.
- [107] Ronald Pethig. Dielectric properties of biological materials: Biophysical and medical applications. *Electrical Insulation, IEEE Transactions on*, (5):453–474, 1984.
- [108] Sami Gabriel, RW Lau, and Camelia Gabriel. The dielectric properties of biological tissues: Iii. parametric models for the dielectric spectrum of tissues. *Physics in medicine and biology*, 41(11):2271, 1996.
- [109] Qammer H. Abbasi, Hassan El Sallabi, Nishtha Chopra, Ke Yang, Khalid Qaraqe, and Akram Alomainy. Terahertz channel characterization inside the human skin at the nano-scale. *IEEE Transactions on THz Science and Technology*, 2016.
- [110] Nishtha Chopra, Akram Alomainy, and Mike Philpot. Investigating electromagnetic material properties of collagen at THz for health monitoring applications. In *MobiHealth 2015*. EAI, 2015.
- [111] Christos Liaskos and Angeliki Tsioliaridou. A Promise of Realizable, Ultra-Scalable Communications at nano-Scale: A multi-Modal nano-Machine Architecture. In *IEEE Transactions on Computers*, pages 1282–1295, 2015.
- [112] Fujitsu. 56GSa/s 8-bit Analog-to-Digital Converter.
- [113] F. Rana. Graphene terahertz plasmon oscillators. *IEEE Transactions on Nanotechnology*, 7(1):91–99, January 2008.

- [114] A. Gupta, M. Medley, and J. M. Jornet. Joint synchronization and symbol detection design for pulse-based communications in the thz band. *submitted for publication*, 2015.
- [115] Jin Tae Kim and Sung-Yool Choi. Graphene-based plasmonic waveguides for photonic integrated circuits. *Optics express*, 19(24):24557–24562, 2011.
- [116] Raul Gomez Cid-Fuentes, J. M. Jornet, Eduard Alarcon, and I. F. Akyildiz. A receiver architecture for pulse-based electromagnetic nanonetworks in the terahertz band. In *Proc. of IEEE International Conference on Communications, ICC*, June 2012.
- [117] C. Han, I. F. Akyildiz, and W. H. Gerstacker. Timing acquisition for pulse-based wireless systems in the terahertz band. In *Proc. of the 2nd ACM International Conference on Nanoscale Computing and Communication (NANOCOM)*, 2015.
- [118] Sheng Xu, Yong Qin, Chen Xu, Yaguang Wei, Rusen Yang, and Zhong Lin Wang. Self-powered nanowire devices. *Nature Nanotechnology*, 5:366–373, 2010.
- [119] J. M. Jornet and I. F. Akyildiz. Joint energy harvesting and communication analysis for perpetual wireless nanosensor networks in the terahertz band. *IEEE Transactions on Nanotechnology*, 11(3):570–580, 2012.
- [120] J. M. Jornet and I. F. Akyildiz. Low-weight channel coding for interference mitigation in electromagnetic nanonetworks in the terahertz band. In *Proc. of IEEE International Conference on Communications (ICC)*, June 2011.
- [121] Murat Kocaoğlu and Ozgur B Akan. Minimum energy channel codes for nanoscale wireless communications. *IEEE Transactions on Wireless Communications*, 12(4):1492–1500, 2013.
- [122] Kaikai Chi, Yi-hua Zhu, Xiaohong Jiang, and Xianzhong Tian. Optimal coding for transmission energy minimization in wireless nanosensor networks. *Nano Communication Networks (Elsevier) Journal*, 4(3):120–130, 2013.
- [123] Kaikai Chi, Yi hua Zhu, Xiaohong Jiang, and V.C.M. Leung. Energy-efficient prefix-free codes for wireless nano-sensor networks using ooh modulation. *IEEE Transactions on Wireless Communications*, 13(5):2670–2682, May 2014.
- [124] N Akkari, JM Jornet, P Wang, E Fadel, L Elrefaei, MGA Malik, S Almasri, and IF Akyildiz. Joint physical and link layer error control analysis for nanonetworks in the terahertz band. *Wireless Networks*, pages 1–13, 2015.
- [125] Pu Wang, J. M. Jornet, MG Abbas Malik, Nadine Akkari, and I. F. Akyildiz. Energy and spectrum-aware mac protocol for perpetual wireless nanosensor networks in the terahertz band. *Ad Hoc Networks (Elsevier) Journal*, 11(8):2541–2555, 2013.
- [126] Shahram Mohrehkesh and Michele C Weigle. Rih-mac: receiver-initiated harvesting-aware mac for nanonetworks. In *Proceedings of ACM The First Annual International Conference on Nanoscale Computing and Communication*, pages 1–9, 2014.
- [127] Q. Xia, Z. Hossain, M. Medley, and J. M. Jornet. A link-layer synchronization and medium access control protocol for terahertz-band communication networks. In *Proc. of IEEE GLOBECOM*, 2015.
- [128] Aria Nosratinia, Todd E Hunter, and Ahmadreza Hedayat. Cooperative communication in wireless networks. *IEEE Communications Magazine*, 42(10):74–80, 2004.
- [129] Aggelos Bletsas, Hyundong Shin, and Moe Z Win. Cooperative communications with outage-optimal opportunistic relaying. *IEEE Transactions on Wireless Communications*, 6(9):3450–3460, 2007.
- [130] I. F. Akyildiz, J. M. Jornet, and Chong Han. Terahertz band: Next frontier for wireless communications. *Physical Communication (Elsevier) Journal*, 12:16 – 32, September 2014.
- [131] Massimiliano Pierobon, J. M. Jornet, Nadine Akkari, Suleiman Almasri, and I. F. Akyildiz. A routing framework for energy harvesting wireless nanosensor networks in the terahertz band. *Wireless Networks*, pages 1–15, 2013.
- [132] Jing Lin, Xiaola Lin, and Liang Tang. Making-a-stop: A new bufferless routing algorithm for on-chip network. *Journal of Parallel and Distributed Computing*, 72(4):515–524, 2012.
- [133] Zheming Zhang, Zhiyang Guo, and Yuanyuan Yang. Bufferless routing in optical gaussian macrochip interconnect. In *IEEE 20th Annual Symposium on High-Performance Interconnects (HOTI)*, pages 56–63, 2012.
- [134] Arun Vishwanath, Vijay Sivaraman, Marina Thottan, and Constantine Dovrolis. Enabling a bufferless core optical network using edge-to-edge packet-level fec. *IEEE Transactions on Communications*, 61(2):690–699, 2013.
- [135] Akbar Ghaffar Pour Rahbar and Oliver WW Yang. Contention avoidance and resolution schemes in bufferless all-optical packet-switched networks: a survey. *IEEE Communications Surveys & Tutorials*, 10(4):94–107, 2008.
- [136] Vuong V Mai, Truong C Thang, and Anh T Pham. Performance of TCP over Free-Space Optical Atmospheric Turbulence Channels. *IEEE/OSA Journal of Optical Communications and Networking*, 5(11):1168–1177, 2013.
- [137] Chong Han, J. M. Jornet, Etimad Fadel, and I. F. Akyildiz. A cross-layer communication module for the internet of things. *Computer Networks (Elsevier) Journal*, 57(3):622–633, 2013.